


## Patient information

Patient ID	095637
Patient Name	-
Accession No.	-

06-04-2022 Processing date

## Patient recommendation

RetCAD outcome More than mild DR detected. Recommendation Patient referral for follow-up testing is advised.




Exam quality: Good



OS RetCAD™ DR assessment: Moderate DR detected 2.67

Exam quality: Good





RetCAD score explanation

Diabetic Retinopathy Relates to the ICDR\* severity classification


- 0: No DR detected
- 1: Mild DR detected
- 2: Moderate DR detected
- 3: Severe DR detected
- 4: Proliferative DR detected
- \* International Clinical Diabetic Retinopathy

## Disclaimers

When more than mild Diabetic Retinopathy (DR  $\geq$  2) is detected, it is recommended to see an eye-care specialist for follow-up diagnosis. The RetCAD software is approved for clinical use and is CE (0344) certified as a Class IIa medical device. The analysis using RetCAD does not replace an eye-health check-up.



## Detailed RetCAD™ analysis results

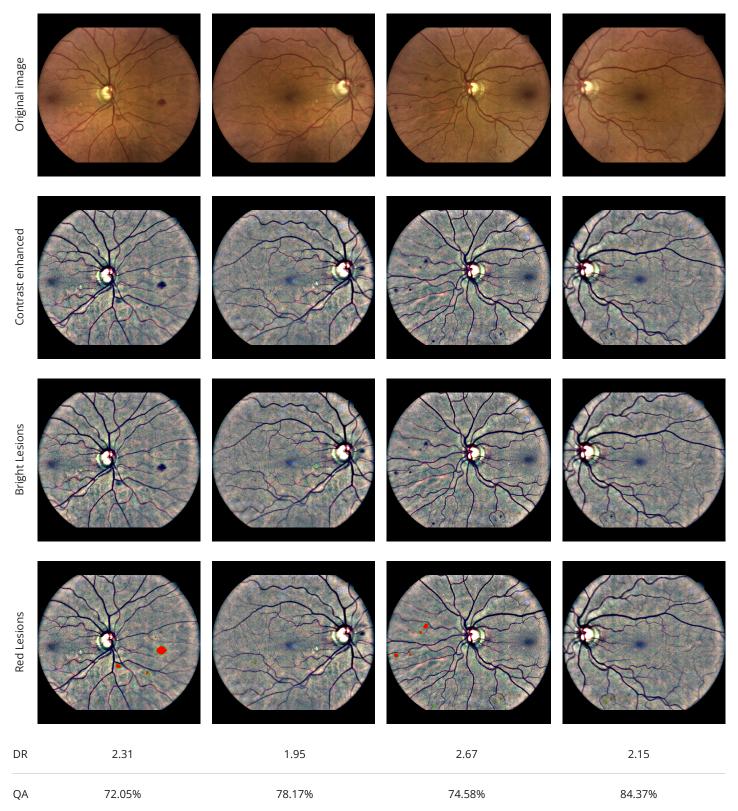

The highest score per disease is taken as the overall eye / patient disease score. Images with a quality assessment (QA) score below 25.00% are deemed insufficient quality and are not taken into consideration for the overall eye / patient assessment. When both images of an eye are deemed insufficient quality, no score is reported for that eye. When an eye is deemed insufficient image quality, no patient score is reported.